

Radiation Protection Survey Map – Room 509


Performed By: Top Notch Tech

Survey Date/Time: less than one week old

Reviewed By: Senior RPT Supervisor

Date: Same day as survey

Location Surveyed: General Areas of Room 509 Buffer Zone and RCA

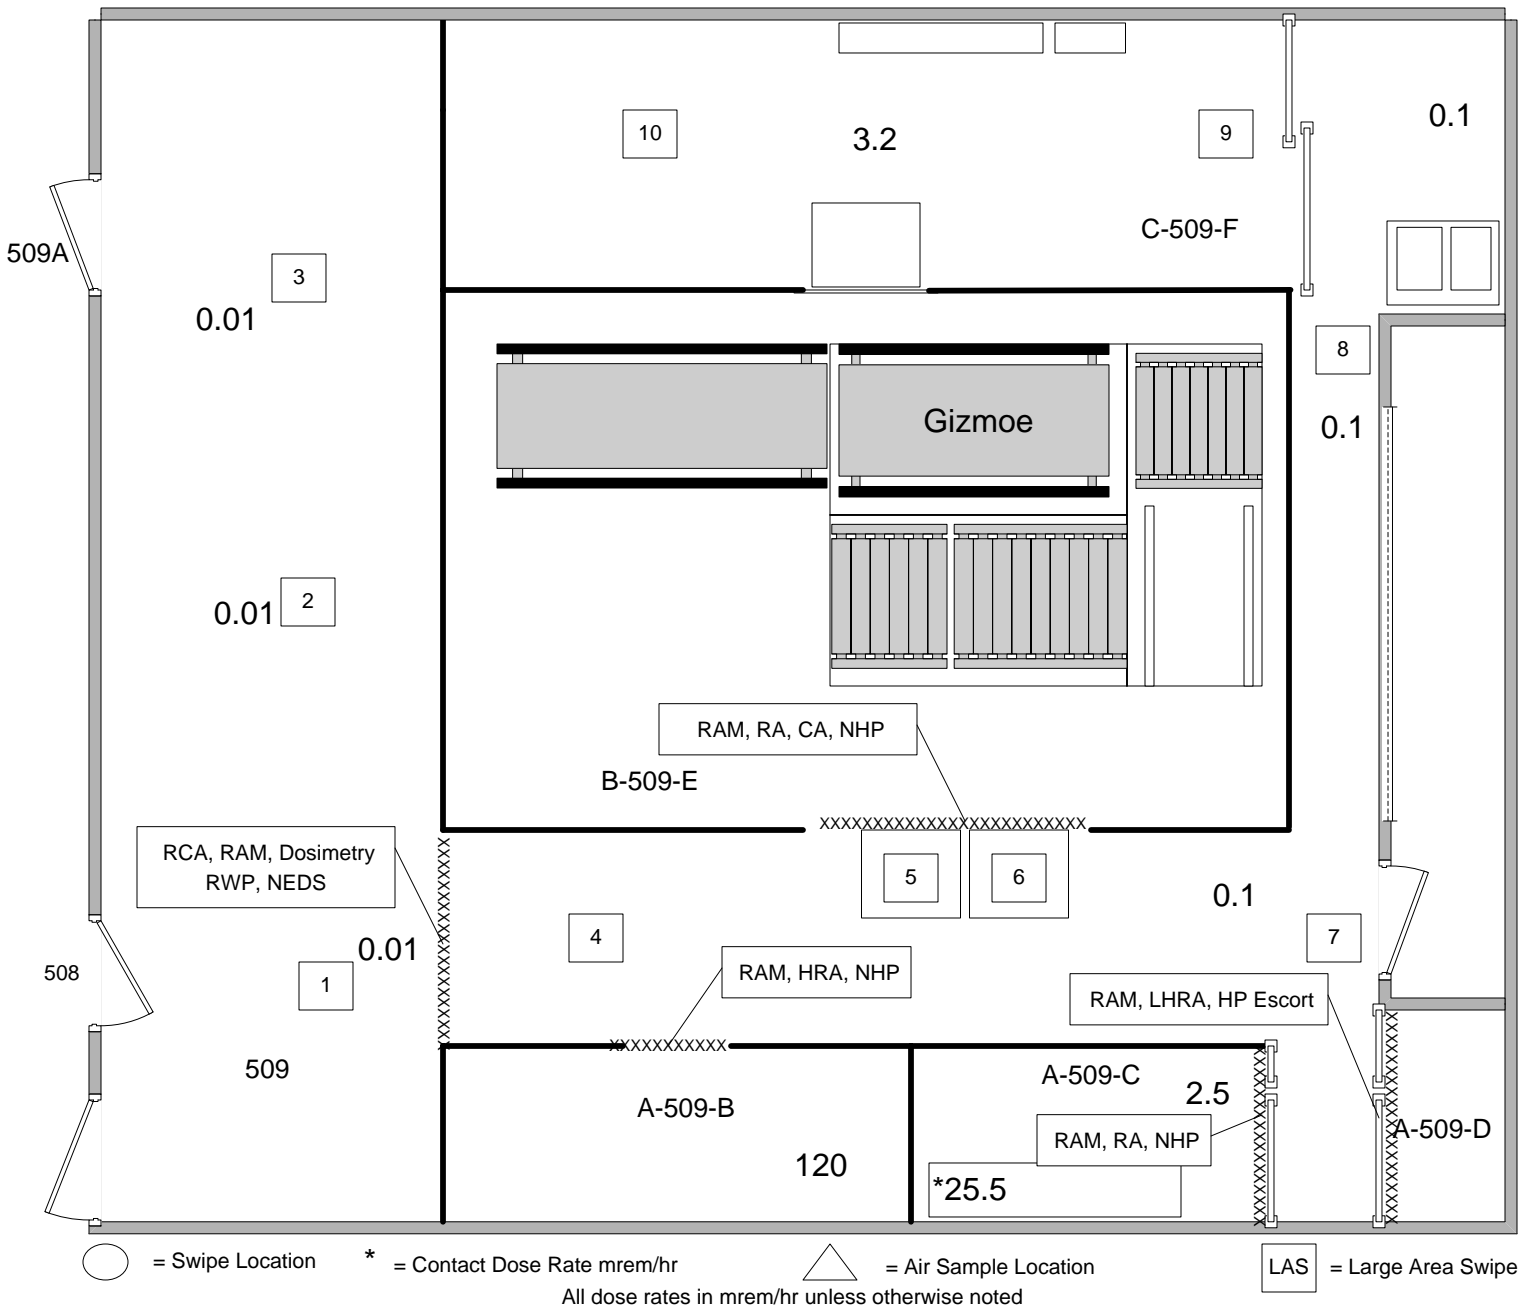

Air Sample
Model: NA
Serial No.: NA
Start LPM: NA
Stop LPM: NA
Radiation Survey Meter
Model: Bicron Micro-R
Serial No.: CMC007845
Cal Due: 1-1-2012
Background: 0.01 mR/hr

Contamination Survey Meter
Model: Ludlum Model 12 w/489-110C
Serial No.: CMC009665
Cal Due: 1-1-2012
Background: 30 cpm

Removable Contamination			
Swipe #	Net cpm	dpm/100 cm ²	Remarks
		All LAS are <100 ccpm	