

Radiation Protection Survey Map – Room 509


Performed By: Samuel Guthrie

Survey Date/Time: one hour old

Reviewed By: Nathan Yarborough

Date: Same day as survey

Location Surveyed: General Areas of Room 509 Buffer Zone and Selected Rooms

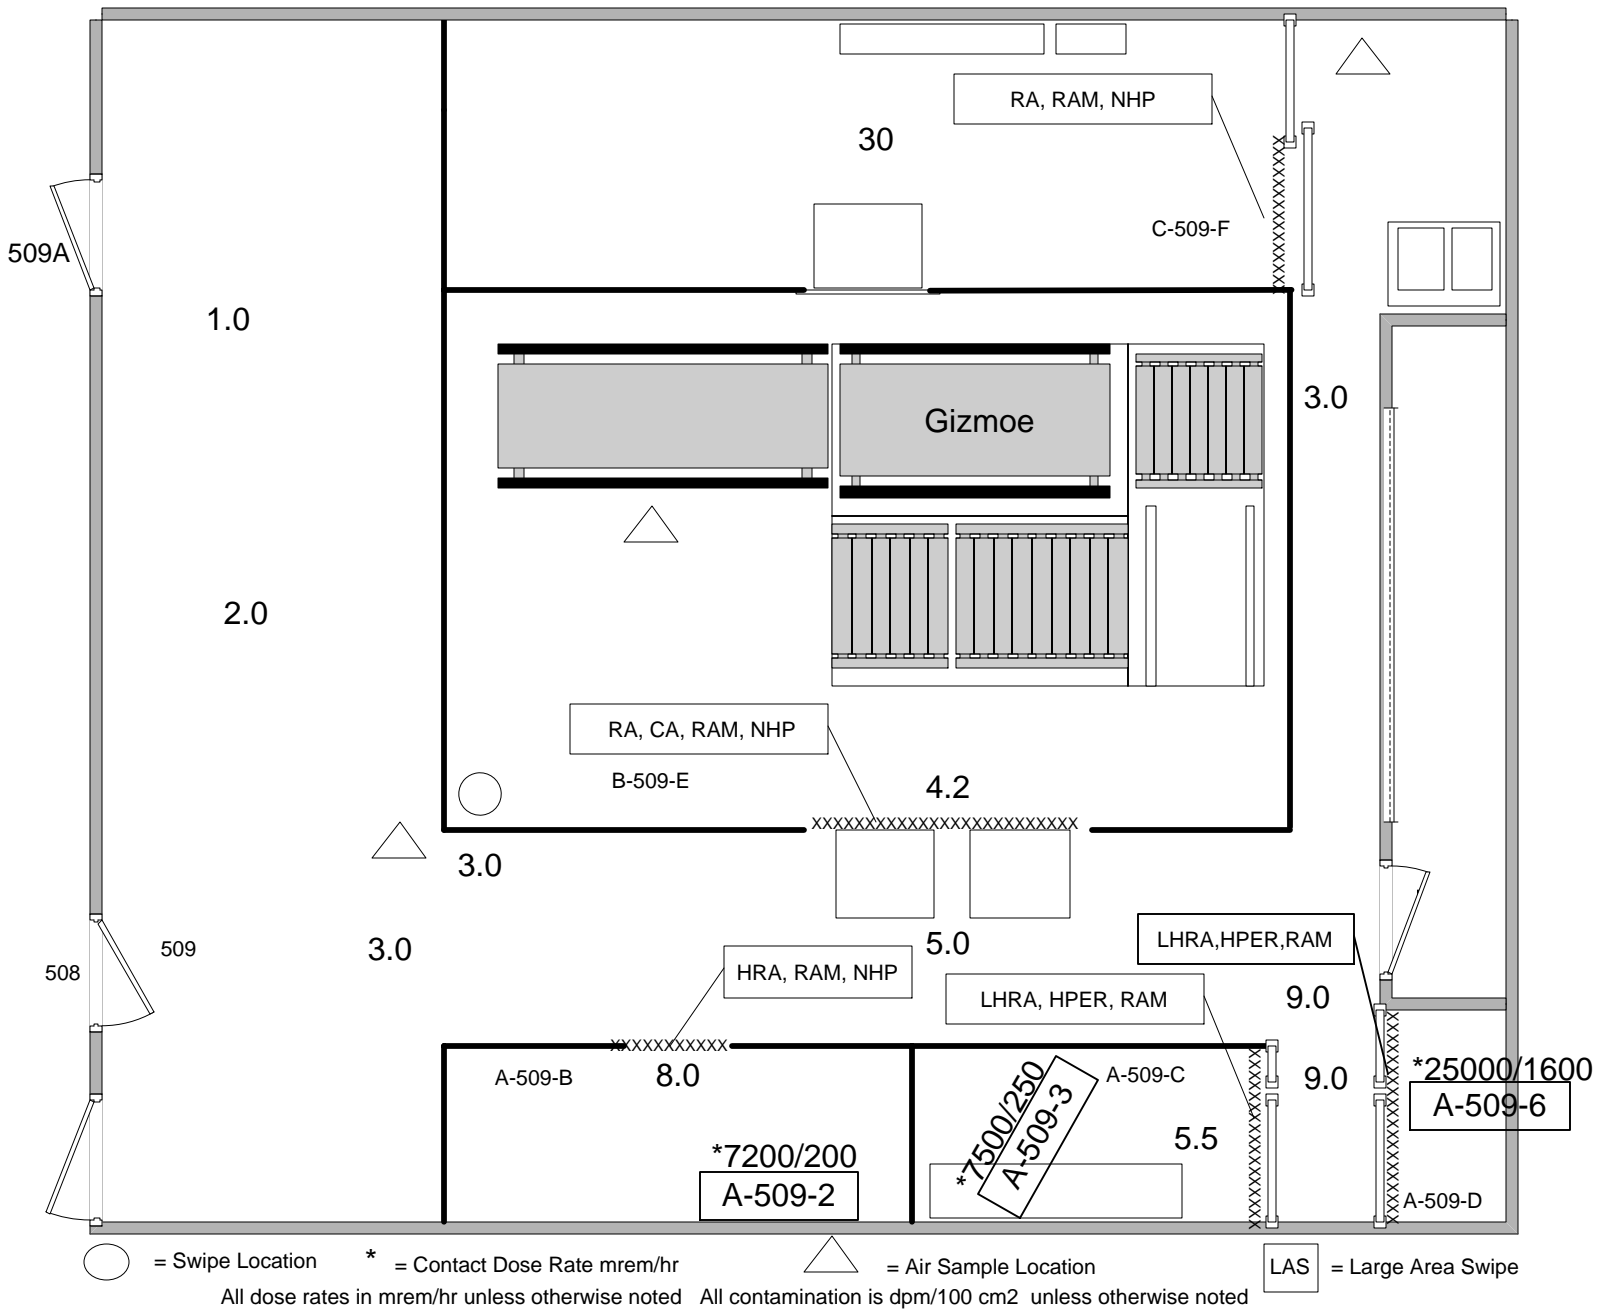

Air Sample
Model: Radeco
Serial No.: 1245 XCA
Start LPM: 75
Stop LPM: 75
Radiation Survey Meter
Model: Bicron Micro-R
Serial No.: CMC007845
Cal Due: 1-1-20x2
Background: 1.0 mR/hr

Contamination Survey Meter
Model:
Serial No.:
Cal Due:
Notes:
Background:

Smear #	Net CPM	dpm	Smear #	Net CPM	dpm
1	NA		10		
2			11		
3			12		
4			13		
5			14		
6			15		
7			NA		
8			NA		
9			NA		